

# NAMING APPARATUS




## SELECT THE CORRECT LEVEL OF MENISCUS



**A**





**B**

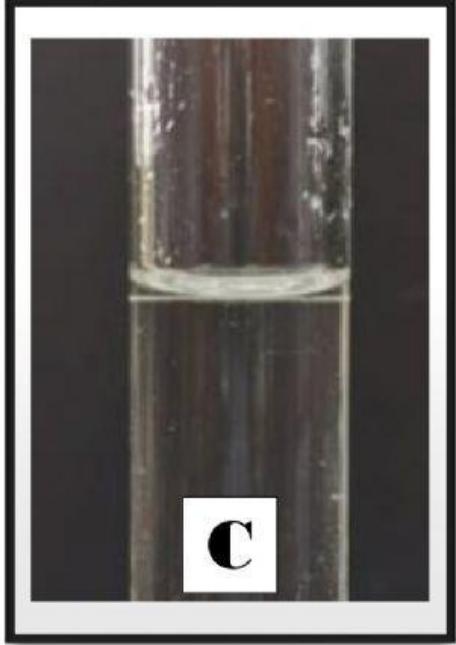

**C**

# BURETTE READING

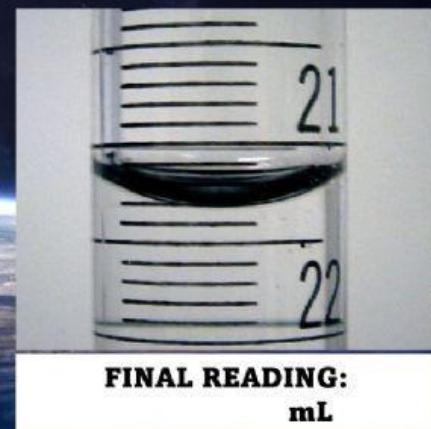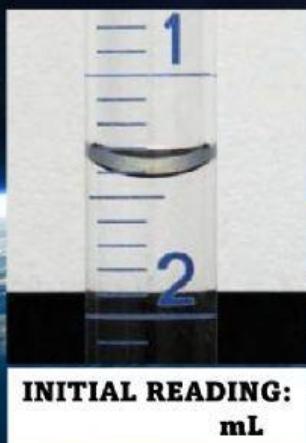

**VOLUME OF SOLUTION USED IN TITRATION:**

**mL**